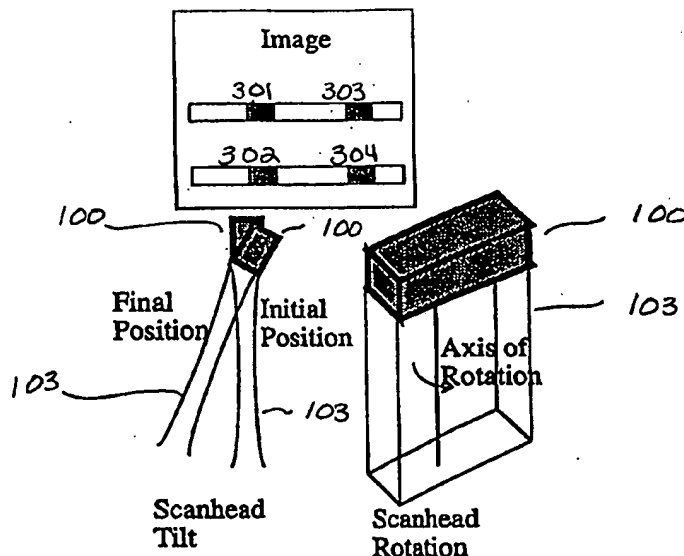## PCT

INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification 6 : G06F 15/00, G06T 15/70	A1	(11) International Publication Number: WO 97/00482 (43) International Publication Date: 3 January 1997 (03.01.97)

(21) International Application Number: PCT/US96/10189

(22) International Filing Date: 14 June 1996 (14.06.96)

(30) Priority Data:
60/000,257   15 June 1995 (15.06.95)   US

(71) Applicant (for all designated States except US): THE REGENT OF THE UNIVERSITY OF MICHIGAN [US/US]; Wolverine Tower, Room 2071, 3003 South State Street, Ann Arbor, MI 48109-1280 (US).

(72) Inventors; and
(75) Inventors/Applicants (for US only): FOWLKES, J., Brian [US/US]; 1425 Saunders Crescent, Ann Arbor, MI 48103 (US). CARSON, Paul, C. [US/US]; 5903 Fow Hollow Court, Ann Arbor, MI 48105 (US). MOSKALIK, Aaron [US/US]; 1066 Island Drive #106, Ann Arbor, MI 48105 (US). CHEN, Jian-Feng [CN/US]; Connemara Apartments #Q201, 3054 230th Lane, S.E., Issaquah, WA 98029 (US). RUBIN, Jonathan, M. [US/US]; 3650 West Huron River Drive, Ann Arbor, MI 48103 (US).

(74) Agent: TOEDT, D., C., III; P.O. Box 4433, Houston, TX 77210 (US).

(81) Designated States: AL, AM, AT, AU, BB, BG, BR, BY, CA, CH, CN, CZ, DE, DK, EE, ES, FI, GB, GE, HU, IL, IS, JP, KE, KG, KP, KR, KZ, LK, LR, LS, LT, LU, LV, MD, MG, MK, MN, MW, MX, NO, NZ, PL, PT, RO, RU, SD, SE, SG, SI, SK, TJ, TM, TR, TT, UA, UG, US, UZ, VN, ARIPO patent (KE, LS, MW, SD, SZ, UG), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, CH, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, ML, MR, NE, SN, TD, TG).

Published
With international search report.

(54) Title: METHOD AND APPARATUS FOR COMPOSITION AND DISPLAY OF THREE-DIMENSIONAL IMAGE FROM TWO-DIMENSIONAL ULTRASOUND

(57) Abstract

A three-dimensional image data set representing a volume of material such as human tissue is created using speckle decorrelation techniques to process successive two-dimensional data slices (301, 302, 303, 304) from a moving, standard 1D or 1.5D ultrasound transducer. This permits the use of standard ultrasound machinery, without the use of additional slice-position hardware, to create 3D images without having to modify the machinery or its operation. Similar techniques can be used for special data processing with the imaging system as well as to expedite the image acquisition process. Optionally, the image quality of 2D images can be enhanced through the use of multiple 3D data sets derived using the method.

1   **METHOD AND APPARATUS FOR COMPOSITION AND DISPLAY OF**

2   **THREE-DIMENSIONAL IMAGE FROM TWO-DIMENSIONAL**

3   **ULTRASOUND**

4

5   The invention described below was made in part with government support. The

6   United States government has certain rights in the invention.

7   As well-known to those of ordinary skill, a standard real-time two-dimensional

8   (2D) ultrasound scan typically entails the following. Referring to Figure 1, an operator

9   holds a transducer 100 in one position relative to a volume of material 102, e.g., human

10 tissue. The transducer 100 is sometimes referred to as a scanhead; it commonly has an

11 essentially linear, one-dimensional (1D) shape, although scanheads of round or other

12 shapes are also known, and emits a beam of ultrasound energy toward the material 102

13 within a "scan plane" 103. The ultrasound energy is reflected from the material 102 and

14 detected by the scanhead, which generates data signals representative of the detected

15 energy. A conventional ultrasound machine 105 receives and processes the resulting

16 data from the scanhead 100 and displays a 2D image of the tissue volume 102 being

17 scanned, e.g., on a video display terminal 107, a film camera, or other hard copy device

18 (not shown). Movement of the scanhead 100 results in different 2D views of the tissue

19 volume 102 being presented.

20   Three-Dimensional (3D) data can be derived from a series of 2D views taken

21 from different angles or positions. These views are sometimes referred to as "slices" of

22 the actual three-dimensional tissue volume 102; the data sets used to generate these

23 views are referred to here as "data slices." Experienced radiologists and similarly

24 trained personnel can often mentally correlate a series of 2D images derived from these

25 data slices to obtain useful 3D information. For example, a radiologist observing a scan

26 of 2D views of a pregnant woman's abdomen may be able to diagnose the fetus's cleft

27 palate by repeatedly moving the scanhead 100 and mentally correlating the 2D images

28 presented.

29   Automated 3D image reconstruction has been done in the past by (a) using

30 mechanical or other means of encoding the successive positions of the scanhead 100 as

1   it is moved about the tissue volume 102, and (b) processing this additional encoded

2   data to provide an indication of the relative positions of the 2D images acquired. This is

3   often difficult to do on a real-time basis. Several technical problems have restricted the

4   use of such systems, including noise interference and limits on spatial resolution. A

5   related approach is to force the scanhead 100 to move over a predetermined track, but

6   that can be adversely affected by movement of the material 102, which often happens in

7   scanning human bodies.

8   Efforts are already being made by some ultrasound scanner manufacturers and

9   others to produce specialized 2D hardware for 3D imaging. Such 2D hardware can be

10   expensive to produce and cumbersome to use, with problems including the current cost

11   and size of the scanhead, image artifacts produced by the fluid path used, etc.

12   Replacing the current 1D arrays with full 2D arrays for making true 3D images is not

13   yet practical due to the number of elements that would be required in the transducer,

14   connections to these and the electronic channels required to services the additional

15   elements.   The ultrasound industry is presently interested in the potential for 3D

16   imaging technology which would not obviate the current cost advantage of 1D

17   scanheads.

18   .   **Speckle Tracking of Moving Tissues**

19   The invention described and claimed below makes a novel use of image

20   analysis, or analysis of RF (radio frequency) data used to create ultrasound images, to

21   indicate the relative position of such images in a three dimensional data set. For

22   example, in one implementation, a speckle correlation technique is used that is well-

23   known in other contexts: When a source of coherent energy (e.g., a laser or an

24   ultrasound beam) interacts with a collection of scatterers, the amplitude of the reflected

25   signal varies in relation to the relative positions of the scatterers. Displayed visually,

26   this amplitude variation appears as a speckle pattern.

27   Ultrasound speckle correlation techniques have been used to determine the

28   movement of blood. Consider an example: Suppose that the material 102 is a human

29   blood vessel with blood cells moving through it. The blood cells are scatterers of the

1   ultrasound energy generated by the scanhead 100, meaning that the amplitudes of the

2   reflected signals vary in relation to the relative positions of the blood cells.

3   The blood cells are continuously circulating in the body, however.

4   Consequently, specific blood cells are continuously moving out from under the

5   scanhead 100 (and out of the ultrasound energy beam) and being replaced by others.

6   As a result, the speckle pattern of the reflected signal is continuously changing

7   because of the movement of the blood cells. This is referred to as "decorrelation" of

8   the signal with respect to the original speckle pattern. By monitoring the amount of

9   decorrelation using standard techniques, the rate at which blood moves under the

10   scanhead may be monitored.

11   The invention described and claimed below was developed in the course of

12   efforts to create 3D images of the breast, to improve the quality of breast cancer

13   diagnosis. It proved difficult to obtain 3D ultrasound images of breasts using

14   conventional mechanical registration of scanhead position. The difficulty was

15   particularly acute for small, dense breasts, which are well recognized as also presenting

16   problems for X-ray mammography diagnosis.

17   In a novel adaptation of decorrelation techniques used for monitoring blood

18   perfusion, a 3D image data set representing a volume of material such as human tissue

19   is created using successive 2D data slices from a moving, standard 1D or 1.5D

20   ultrasound transducer. (The term "1.5D" refers to the use of a limited number of

21   separate elements in a second dimension.) This permits the use of standard ultrasound

22   machinery, without the use of additional slice-position hardware, to create 3D images

23   without having to modify the machinery or its operation. Similar techniques can be

24   used for special data processing within the imaging system as well to expedite the

25   image acquisition process.

26   Optionally, the image quality of 2D images can be enhanced through the use of

27   multiple 3D data sets derived using the method.

28   Figure 1 is a simplified perspective view of an ultrasound scanner being used to

29   scan a material.

1   Figure 2 is a flow chart depicting the operations performed in a method in

2   accordance with the invention.

3   Figure 3 illustrates a method of monitoring scanhead tilt and rotation.

4   Figure 4 illustrates an approach to scanhead position tracking.

5   Figure 5 depicts an approach to slice positioning.

6   Figure 6 is a block diagram of software modules used in one implementation of

7   the invention.

8   **A Post-Processing Implementation**

9   An illustrative implementation of a method in accordance with the invention is

10   depicted in flow-chart form in Figure 2. At block 200, data acquired by ultrasound

11   scanning of a material 102 using a scanhead 100 are collected into a computer memory

12   for post-processing by a computer or other machine, e.g., by a programmable

13   ultrasound machine 105 loaded with a suitable computer program or programs. The

14   material in question may be a volume of human tissue or any other material suitable for

15   ultrasound scanning, as well known in the art.

16   The scanning process itself generates a series of signals encoding data

17   representing physical two-dimensional "slices" of the material being scanned. At block

18   205, data encoded in signals corresponding to the respective slices of the material are

19   defined and referred to for convenience as data slices. One or more regions is defined

20   within a first data slice, referred to as data slice 1. Similarly, one or more regions is

21   defined within another data slice, referred to as data slice 2.

22   At block 210, the amounts of correlation between the respective regions in data

23   slice 1 and data slice 2 are conventionally determined. For example, suppose that data

24   slice 1 is divided into regions 1a, 1b, etc., and data slice 2 is divided into regions 2a, 2b,

25   etc. The amount of correlation between regions 1a and 2a is determined, as is the

26   amount of correlation between regions 1b and 2b, etc. The respective amounts of

27   decorrelation may be determined by a process of speckle decorrelation measurement as

28   known to those of ordinary skill.

1   At block 215, the respective amounts of correlation between the regions are

2   used to compute, in conventional fashion, a relative positional difference vector that

3   represents a relative positional difference between data slice 1 and data slice 2. Those

4   of ordinary skill having the benefit of this disclosure will recognize that the relative

5   positional difference vector could be a scalar, i.e., a one-dimensional vector.

6   Data representations of at least a portion of data slice 1, at least a portion of

7   data slice 2, and the computed relative positional difference vector may be stored in a

8   memory device, e.g., RAM or a disk storage device in a computer, for future use.

9   Those of ordinary skill having the benefit of this disclosure will recognize that the data

10   representations may be preprocessed if desired before storage, e.g., by conventionally

11   "compressing" the data for greater storage efficiency. Such compression might

12   include, e.g., storing, as the representation of a given data slice, a vector representing a

13   change from a different data slice. Other compression techniques such as the well-

14   known LZW method may also be used.

15   At block 220, from the relative positional difference vector, a computation is

16   made to determine the relative positions of data slice 1 and data slice 2 within a 3D

17   image of the material. The 3D image is conventionally displayed on a visual display

18   such as a video display terminal, a computer printout, a computer-generated

19   photograph, etc.

20   Optionally, portions of the data slices may be processed as described above

21   instead of the entire data slices. That is, the portions acquired and processed may be of

22   sizes smaller than is necessary to create a complete 2D image. Processing of such

23   smaller portions may be used to determine the scanhead position.

24   The foregoing operations are discussed in more detail below.

25   **Scanning the material volume**

26   The material volume 102 in question is conventionally scanned with any

27   standard ultrasound scanner, using a linear scan for coverage of a comparatively large

28   region, optionally with a tilt of the scanhead 100 to get at hard-to-reach places, e.g.,

29   under the rib cage in the case of medical scanning. The image data thereby obtained

1   during the scan may be conventionally collected in any of a variety of forms, i.e.

2   envelope-detected, RF, etc.

3   Optionally, a rotational scan may be used to image an area under the transducer

4   in the volume of rotation. (The volume immediately adjacent to the transducer's

5   starting position may be included in the rotation.) This provides at least two

6   advantages: First, rotating the scanhead about a central scan-line axis allows repeated

7   views of the same portions of the material volume, which helps correct for any

8   scanhead movement that may occur. Second, when the scanhead is rotated,

9   decorrelation occurs at different rates along the radius out from the axis of rotation

10 (i.e., the radius of the circle of rotation), allowing a more rapid image acquisition. A

11 disadvantage, of course, is that the scan area is only as big as the area scanned by

12 having the axis of rotation at one end of the scanhead.

13   More than one set of 3D image data may be obtained from different scanning

14 directions. These may be combined by one or more methods discussed below (cross

15 correlation between vertical scan lines and homologous point registration) to position

16 the images with respect to each other. Although orthogonality of the 3D image data is

17 not required, if two sets of 3D image data are orthogonal then each image in one set

18 where the geometry is fixed within the scan plane provides maximal information to aid

19 in positioning the planes in the other data set.

20   **Determining relative decorrelation of specific portions of the image**

21   A region of interest is defined in one of the data slices in the series of data

22 slices. A corresponding region of interest is defined on a second slice. The second slice

23 may be immediately adjacent the first slice (e.g., slices 1 and 2) or more widely spaced

24 from the first slice (e.g., slices 1 and 3), depending on the desired sampling rate for the

25 implementation in question.

26   The amount of correlation between the two corresponding regions of interest is

27 experimentally measured, using conventional techniques, and compared to previously-

28 measured decorrelation for a given transducer. The decorrelation measured may be

29 related to the type of the material 102 as necessary to improve accuracy. The

1   measured decorrelation permits conventional computation of the relative positional

2   difference between the two slices. The same computations are performed for each

3   successive pairs of slices.

4   As shown in Figure 3, the tilt and rotation of the transducer or scanhead 100

5   may be monitored by examining the decorrelation rates at various positions of the

6   scanhead within the scan plane. Assume, for example, two specified regions of the

7   material 102 at differing distances from the scanhead 100. If the decorrelation rates

8   differ after appropriate corrections for the beam shape, then it follows that the scanhead

9   100 is being tilted as shown in Figure 3. By examining the difference between two

10   regions separated in the lateral direction, rotation of the scanhead may be monitored

11   regardless of where the rotation axis was in the lateral direction. In Figure 3, the

12   difference in rate between regions 301 and 302 and between 303 and 1 indicates tilting

13   of the scanhead. By examining differences in the lateral direction, i.e. differences

14   between 301 and 303 and between 302 and 304, rotation of the scanhead may be

15   monitored regardless of where the rotation axis was in the lateral direction.

16   When two data sets from differing look directions are obtained, one method

17   which may be used to position the scan planes in one set is to use the position of the

18   intersection between every pair of scan planes as shown in Figure 5. This is

19   accomplished by performing a cross correlation between vertical scan lines from each

20   data set (referred to as "A mode correlation). The peak of this correlation defines the

21   intersection of the two planes and any relative vertical movement between the planes.

22   These correlation values are then mapped onto a 2D representation of the area near the

23   intersection. The position of the peak value in this 2D area is the estimated position of

24   the intersection, which defines the position of both planes. The magnitude of this peak

25   relative to the rest of the 2D area can be used as a weighting. Each plane's position

26   will be estimated by using all of its intersections with the orthogonal image. Its final

27   position is determined, then, by the weighted average of these estimates. In this way, a

28   strong feature found on the intersection of two scan planes contributes heavily to the

29   determination of their positions.

1   Another method which may be applied to any nonparallel image sets taken

2   within the same volume of material is the use of homologous points registration.

3   Points or other structures which can be identified as common to two or more data sets

4   can be used to correctly define the geometric relationship between the image sets. In

5   the case of two orthogonal planes, the process is quite simple. The images are first

6   placed with some arbitrary spacing. As noted in subpart 4.1B above, the geometric

7   relationship within an image (x-z plane of one 3D data set) is known. Therefore if

8   objects identified within an image plane can be similarly identified in the reconstructed

9   x-z plane of the other set then the image plane separation and the vertical position of

10 the image planes can be adjusted to correctly position the plane. The difficulty with the

11 method as described is the need for manual or electronic identification of homologous

12 points.

13   Once the methods described in subparts 4.1A, B, or C are complete,

14 conventional image-processing techniques are used to position the data slices, utilizing

15 the relative-position information obtained above to correctly position each data slice in

16 a 3D display, which can then be output to a monitor, a hard copy, etc. Optionally, the

17 data slices can be interpolated to produce a 3D image data set with uniform spacing.

18   Those of ordinary skill having the benefit of this disclosure will appreciate that

19 multiple 3D data sets acquired in this fashion can be conventionally processed to

20 improve the overall image quality of the 2D slices in the 3D sets. Those 2D slices can

21 be redisplayed as two-dimensional images if desired.

22   **On-the-Fly Processing**

23   It is anticipated that in another implementation, by restricting the regions that

24 are measured for motion, it will be possible to minimize the computational time to the

25 point where such monitoring can be performed in real-time. The advantage is that the

26 position information may be computed at a rate faster than the frame rate of the

27 imaging system. Also, it is expected to be possible to set motion criteria which will

28 indicate when the images should be taken to provide an automated way of reducing the

29 number of frames acquired in the 3D data set and fix their spacing to make

1   reconstruction simpler. The processing of RF data for position encoding would then be

2   a separate process which is expected to be more accurate than that possible for the

3   envelope-detected information. In addition, the decorrelation as calculated by these

4   methods may be used to measure the velocity of the scanhead and provide the operator

5   an indication to gauge the rate at which the material should be scanned.

6   **Some Additional Implementations of the Invention**

7   The benefits of eliminating the requirement for encoding of scanhead-position

8   data should not be underestimated. It will be apparent to those of ordinary skill having

9   the benefit of this disclosure that in addition to the elimination of cumbersome

10 manipulation systems and/or position encoding devices, an image-based slice

11 positioning system can provide other motion artifact reduction possibilities and similar

12 capabilities.

13   For example, it is expected that speckle decorrelation techniques of the kind

14 described above can be used for the correction of respiratory motion when 3D data set

15 is reconstructed. Elevational correction as described above as well as in-plane

16 correction can be used to keep a region of interest stationary in the image.

17   As another example, it is expected that acquisition of multiple planes, e.g., two,

18 at each location, and correlation of subsequent frames with these can be used to

19 determine when the transducer has moved a fixed distance. This enables not only

20 knowledge of distance traveled but also direction. Figure 4 depicts how the technique

21 may be applied. At Position 1 two scan planes 103 from a so-called 1.5D scanhead

22 array 400 (which is divided into two linear arrays or potentially used to steer into a

23 second scan plan) are formed at positions 401 and 402. Subsequently the transducer or

24 scanhead moves and as the images are acquired the correlation is calculated. A peak

25 correlation will occur between the previously acquired scan plane 402 and the new

26 plane at position 403 when the scanhead has moved a fixed distance. Note that

27 correlations can be made also for motion in the opposite direction. The placement of

28 planes in the 3D data set could be performed only when the correlation occurred thus

29 placing the planes on a uniform grid space. Or if more planes were needed, the planes

1   which were acquired between correlation points could be spaced uniformly over the

2   distance traveled.

3   The rate that the speckle pattern is changing can also indicate the presence of

4   phase aberrators in the field of view for the scanhead. By looking at various regions of

5   the image, sudden, inconsistent, regional changes in correlation rates will indicate an

6   aberration of phase. Such mapping could indicate which data to throw out of some

7   images when compounding or reconstructing in 3D or perhaps when and where phase

8   aberration correction would need to be performed in the images.

9   It is anticipated that the above described techniques can also be used for fine

10   positioning of a scanhead in conjunction with other positioning systems. The latter

11   might be able to monitor the long range motion of the scanhead but lack the fine spatial

12   resolution required for the best 3D reconstructions. Such encoding devices include

13   optical, mechanical, magnetic, electric spark systems, etc. all of which have been used

14   in the past for 3D ultrasound imaging.

15   It is also anticipated that 2D speckle tracking (Chen, Hein et al. 1991; Chen,

16   Jenkins et al. 1992) can be used to monitor motion in the scan plane between adjacent

17   slices and then measure the decorrelation result. In such an implementation, the 2D

18   speckle tracking identifies the correct vertical and horizontal translation required for

19   placing the adjacent slice with respect to the first. The minimum decorrelation value is

20   determined by comparing selected regions in the two images and the relative positions

21   of the location with minimum decorrelation would indicate the relative vertical and

22   horizontal position of the planes. The minimum decorrelation value which then

23   remained between the slices is the result of the translation in the elevational direction

24   and is expected to be an improved estimate over assuming no vertical or horizontal

25   motion.

26

27   **Software**

28   Figure 6 is a block diagram of preliminary software as implemented under the

29   AVS software package of Advanced Visualization Systems of Waltham,

30   Massachusetts. Images are collected from an ultrasound scanner and read into the

1   workstation memory. In this example the data is obtained using a TARGA frame

2   grabber and thus the module TGA Stacker 600 is used. The RGB images are then

3   processed by extract scalar 605 to select one channel and then the 3D data set is sliced

4   using orthogonal slicer 610 and a single 2D plane displayed using image viewer 615 to

5   select regions of interest (ROIs) to be processed for determining the slice separation.

6   The region is selected using crop 620 and redisplayed using another image viewer 625.

7   The pixels contained in the ROI in each image is converted to a 1D vector using ROI

8   to strip 630 and the process repeated using animated integer 635 connected to the

9   orthogonal slicer 610. Each of these strips are then combined in a 2D vector using glue

10 640. These data are then subsampled using another crop 645 to determine the how

11 many of the image ROIs will be used to compute the position of each image. The

12 controls for determining which images are processed for each slice position calculation

13 are contained in animated integer 650, generate integer 655, and integ_math 660. The

14 cropped output is then analyzed by the correlate module 665 which computes the

15 correlation between successive ROIs, i.e. ROI#1 correlation to ROI#2, ROI#2 to

16 ROI#3, etc. for a one step correlation value. The process is repeated for two, three,

17 etc. step correlations. The correlation curve is then fitted to determine the slice

18 separation for the center two slices in the set used to measure the decorrelation rate.

19 The output of this correlator is displayed by the graph viewer 670 and saved as a file

20 which contains a separation value between each image and the next. This information

21 is then read into fld2rect module 675 and the images from the TGA Stacker 600 are

22 correctly spaced. The correctly positioned images can then be displayed by any desired

23 means such as the ortho 3 slices 680 and geometry viewer 685.

24

25   **Additional Considerations**

26   In a simple implementation, one can use a sequence of three normally obtained

27 data slices which do not rely on a special transducer construction. In this scenario, the

28 first data slice is obtained and then the second and third as the transducer is translated

29 over the object being imaged. Using the first data slice as a reference, the second data

30 slice will be slightly decorrelated from the first due to transducer motion. If the motion

1   continues in the same direction then the decorrelation that exists between the third data

2   slice acquired and the first will be larger than that between the second and third data

3   slice.   If however, the direction changes after data slice 2 is obtained, i.e., the

4   transducer moves back toward the position of data slice 1, then the correlation will be

5   greater between data slices 1 and 3.

6   The inclusion of specific portions of data slices has significance in at least two

7   ways. First, the selection of data to be used in the positioning of slices can contribute

8   to the success of the positioning. For example, the inclusion of specular reflectors will

9   cause the decorrelation rate to change (slow down) in a manner not related to the

10 transducer motion. Therefore it is helpful to know the characteristics of the material

11 producing the speckle pattern so that the decorrelation of this speckle can be used to

12 determine the position of slices. Second, conventional criteria can be used to produce

13 images of specific tissue types and characteristics or in the compounding of multiple

14 sets of data slices to produce improved images as in the case of speckle reduction or

15 imaging of connective tissue (specular reflectors).

16

CLAIMS:

1   1.   A method, executed by a machine, of displaying a 3D image of a human tissue
2   volume, said method comprising:

3   (a)   receiving a plurality of data sets, referred to as data slices, each said
4   data slice representing a respective 2D slice of said tissue volume, said
5   plurality of data slices having been generated by ultrasound scanning of
6   said tissue volume;

7   (b)   defining (1) one or more regions within one of said data slices, referred
8   to as regions 1a, 1b, and so on, within data slice 1, and (2) one or more
9   regions within another of said data slices, referred to as regions 2a, 2b,
10   and so on, within data slice 2;

11   (c)   performing a process of speckle decorrelation measurement to
12   determine respective amounts of correlation between regions 1a and 2a,
13   regions 1b and 2b, and so on;

14   (d)   utilizing said respective amounts of correlation to compute a relative
15   positional difference vector representative of a relative positional
16   difference between data slice 1 and data slice 2;

17   (e)   writing to said memory (1) a representation of at least a portion of said
18   data slice 1, (2) a representation of at least a portion of said data slice 2,
19   and (3) said relative positional difference vector;

20   (f)   computing, from said relative positional difference vector, a relative
21   position of each of said data slice 1 and said data slice 2 within a 3D
22   image of the material; and

23   (g)   displaying said 3D image on a visual display.

24

1   2.   A method, executed by a machine, of creating a memory containing a data
2   structure encoding a series of two-dimensional representations of a material,
3   said method comprising:

4   (a)   receiving a plurality of data sets, referred to as data slices, each said

5   data slice representing a respective slice of said material;

6   (b)   defining (1) one or more regions within one of said data slices, referred

7   to as one or more regions within data slice 1, and (2) one or more

8   regions within another of said data slices, referred to as one or more

9   regions within data slice 2;

10   (c)   measuring respective amounts of correlation between said one or more

11   regions within data slice 1 and said one or more regions within data slice

12   2;

13   (d)   utilizing said respective amounts of correlation to compute a relative

14   positional difference vector representative of a relative positional

15   difference between data slice 1 and data slice 2; and

16   (e)   writing to said memory (1) a representation of at least a portion of said

17   data slice 1, (2) a representation of at least a portion of said data slice 2,

18   and (3) said relative positional difference vector.

19

1   3.   The method of claim 2, wherein at least some of said data slices are smaller in

2   size than required to specify a two-dimensional image.

3

1   4. The method of claim 2, wherein said data slices are received from a scanhead having

2   a position relative to the material, and further comprising determining said

3   position by performing a computation utilizing respective portions of at least

4   two of said data slices.

5

1   5.   The method of claim 2, wherein said data slices are received from a scanhead

2   that is being moved relative to the material at a rate referred to as a scanning

3   rate, and further comprising determining, from respective portions of at least

4   two of said data slices, one or more of (i) a total number of data slices to be

5   acquired, and (ii) a desired scanning rate.

6

1   6.   The method of claim 2, wherein :

2   (1)   at least some of said plurality of data slices are generated by scanning at

3   least a portion of said material with a beam of coherent energy; and

4   (2)   said material comprises a plurality of energy scatterers.

5

1   7.   The method of claim 6, wherein said energy scatterers reflect coherent energy in

2   a speckled pattern.

3

1   8.   The method of claim 2, further comprising:

2   (1)   computing, from said relative positional difference vector, a relative

3   position of each of said data slice 1 and said data slice 2 within a 3D

4   image of the material; and

5   (2)   displaying said 3D image on a visual display.

6

1   9.   The method of claim 2, wherein said measurement of respective amounts of

2   correlation is performed by a process of speckle decorrelation measurement.

3

1   10.   The method of claim 2, wherein said 2D data slices are generated by an

2   ultrasound scan of said material.

1   11.   The method of claim 2, wherein said material is a tissue volume.

2

1   12.   The method of claim 2, wherein

2   (1)   said measurement of an amount of correlation between a first one of

3   said one or more regions in data slice 1 and a region in data slice 2 is

4   performed by (i) locating one of said one or more regions in data

5   slice 2 that has a minimum decorrelation value, referred to as a

6   minimum-decorrelation region, and (ii) determining two orthogonal in-

7   plane components of a vector between said minimum-decorrelation

8   region and said first one of said regions in data slice 1; and

9   (2)   said utilization of said amount of correlation is performed by utilizing, as

10   said measurement of said amount of correlation, an out-of-plane

11   component of said vector that is orthogonal to said in-plane

12   components.

13

1   13.   A method, executed by a machine, of displaying a 3D image of a human tissue

2   volume, said method comprising:

3   (a)   receiving a plurality of data sets, referred to as data slices, each said

4   data slice representing a respective 2D slice of said tissue volume;

5   (b)   defining (1) one or more regions within one of said data slices, referred

6   to as one or more regions within data slice 1, and (2) one or more

7   regions within another of said data slices, referred to as one or more

8   regions within data slice 2;

9   (c)   performing a process of speckle decorrelation measurement to

10   determine respective amounts of correlation between said one or more

11   regions in data slice 1 and said one or more regions in data slice 2;

12   (d)   utilizing said respective amounts of correlation to compute a relative

13   positional difference vector representative of a relative positional

14   difference between data slice 1 and data slice 2;

15   (e)   computing, from said relative positional difference vector, a relative
16   position of each of said data slice 1 and said data slice 2 within a 3D
17   image of the material; and
18   (f)   displaying said 3D image on a visual display.

19

1   14.   A program storage device readable by the machine of a specified one of claims
2   1 through 13, encoding instructions for performing the operations of said
3   specified one claim.

4

1   15.   A machine containing a memory having a data structure created by a method in
2   accordance with a specified one of claims 2 through 12.

3

1   16.   A method in accordance with claim 2, wherein said data slices are obtained
2   using an imaging transducer.

3

1   17.   A method in accordance with claim 16, further comprising:
2   determining that motion of said transducer has changed by detecting an increase
3   in the correlation of at least one data slice relative to at least one other
4   previously obtained data slice.

5

1   18.   A method in accordance with claim 2, wherein said step of computing said
2   relative positional difference vector comprises image processing to find regions
3   of coherent speckle.

4

1   19.   A method in accordance with claim 2, wherein said step of computing said
2   relative positional difference vector comprises image processing to extract data
3   which do not represent coherent speckle.
4

1   20.   A method in accordance with claim 2, wherein said step of computing said
2   relative positional difference vector comprises image processing to extract data
3   which do not decorrelate rapidly.
4

1   21.   A method in accordance with claim 2, wherein said step of computing said
2   relative positional difference vector using characteristics of data in a data slice
3   to predict the behavior in an out-of-plane direction to include data in the
4   positioning of slices.
5

1   22.   A method in accordance with claim 2, wherein said step of computing said
2   relative positional difference vector comprises using characteristics of data in a
3   data slice to predict the behavior in an out-of-plane direction to exclude data in
4   the positioning of slices.
5

1   23.   A method of generating image views of imaged material, which views reveal
2   specific characteristics of said material, comprising:
3   (a)   receiving a plurality of data sets, referred to as data slices, each data
4   slice representing a respective 2-D image of said material;
5   (b)   image processing said data slices to identify regions of coherent speckle
6   therein;
7   (c)   generating said image views using slices having regions of coherent
8   speckle therein.
9

1   24.   A method of generating image views of imaged material, which views reveal
2   specific characteristics of said material, comprising:
3

4   (a)   receiving a plurality of data sets, referred to as data slices, each data
5   slice representing a respective 2-D image of said material;
6   (b)   image processing said data slices to extract data which do not represent
7   coherent speckle;
8   (c)   generating said image views using said processed data slices.

9

1   25.   A method of generating image views of imaged material, which views reveal
2   specific characteristics of said material, comprising:
3   (a)   receiving a plurality of data sets, referred to as data slices, each data
4   slice representing a respective 2-D image of said material;

5

6   (b)   image processing said data slices to assess decorrelation rates in 3-D;

7

8   (c)   selecting data slices for said image views based on said assessed
9   decorrelation rates.

10

1   26.   A method in accordance with claim 24, wherein said step (b) of image
2   processing to extract data which do not represent coherent speckle comprises
3   detecting and subtracting data corresponding to reverberations.

4

1   27.   A method in accordance with claim 25, wherein said step (c) of selecting data
2   slices based on assessed decorrelation rates comprises assessing decorrelation
3   rates in adjacent slices to identify sets of slices in which decorrelation rate
4   corresponds to artifacts of multiple scattering, refraction, diffraction, or
5   shadowing.

6

1   28.   A method in accordance with claim 25, wherein said step (c) of selecting data
2   slices based on assessed decorrelation rates comprises assessing decorrelation
3   rates in adjacent slices to identify regions of adjacent slices decelerating more
4   rapidly than remaining regions in said adjacent slices.

5

1 29.   A method in accordance with any of claims 26, 27, or 28, further comprising
2   the step (d) of generating image views using data slices and portions of data
3   slices which are relatively free from artifact.

4

1 30.   A method in accordance with any of claims 26, 27, or 28, further comprising
2   the step (d) of generating image views using data slices which reveal a desired
3   characteristics of said imaged material.

4

1 31.   A method in accordance with claim 2, wherein said plurality of data sets
2   include data slices from at least two different look directions.

3

1 32.   A method in accordance with claim 31, wherein all but one of said plurality of
2   data sets can include only one data slice.

3

1 33.   A method in accordance with claim 32, further comprising the step (f) of
2   spatially aligning said plurality of data sets.

3

1 34.   A method in accordance with claim 33, further comprising the step (g) of
2   refining said relative positional difference vectors between adjacent slices.

3

1 35.   A method in accordance with claim 34, wherein said step (f) of spatial
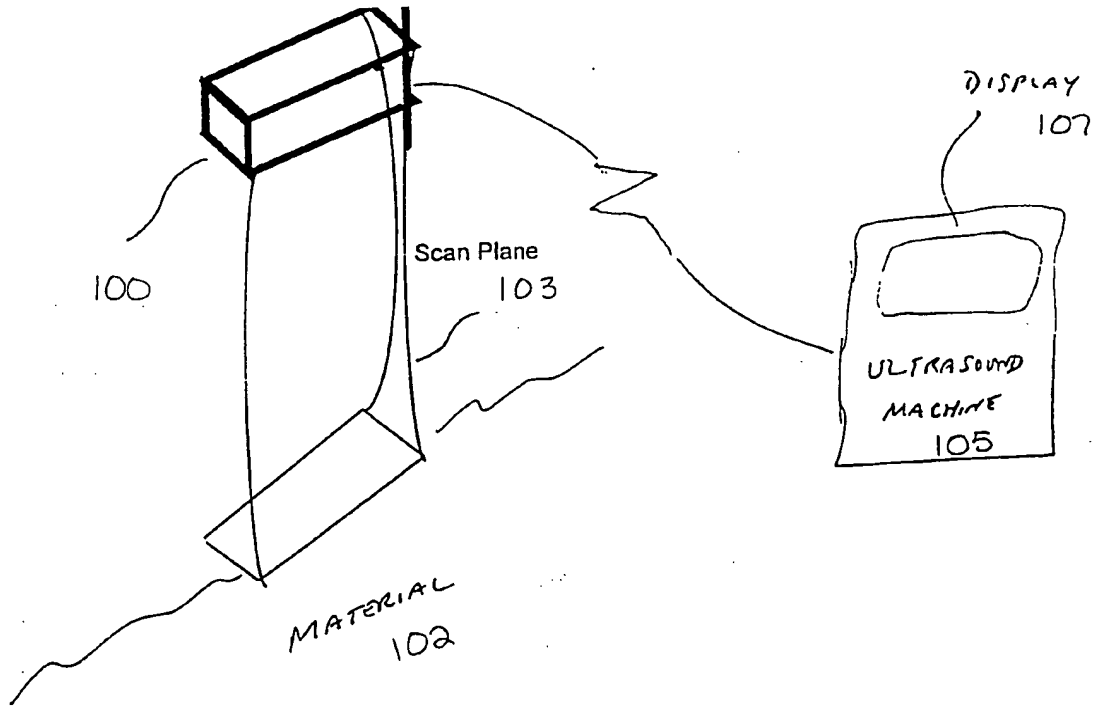2   alignment further comprises the steps of:
3   (h)   of cross-correlating comparisons of vertical lines between two data sets
4   to locate a most likely intersection point of two data slices from said
5   two data sets; and

6

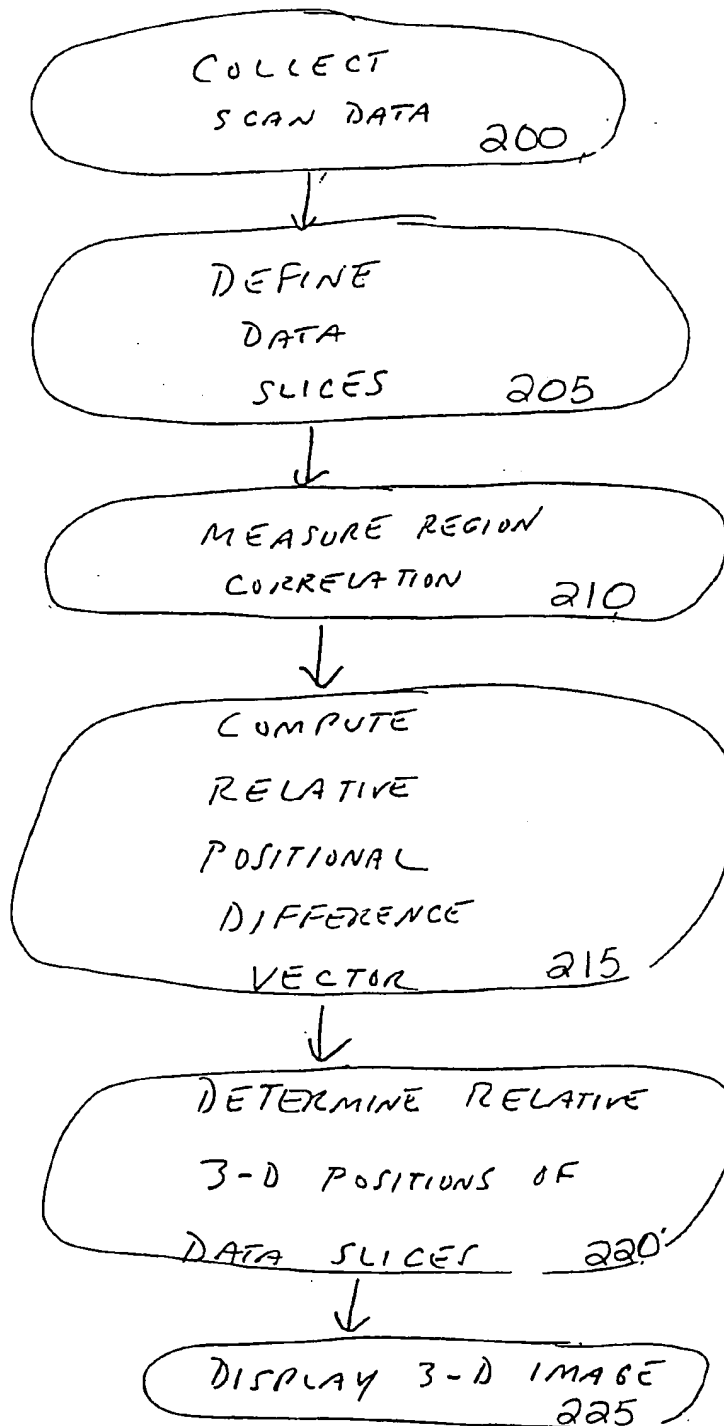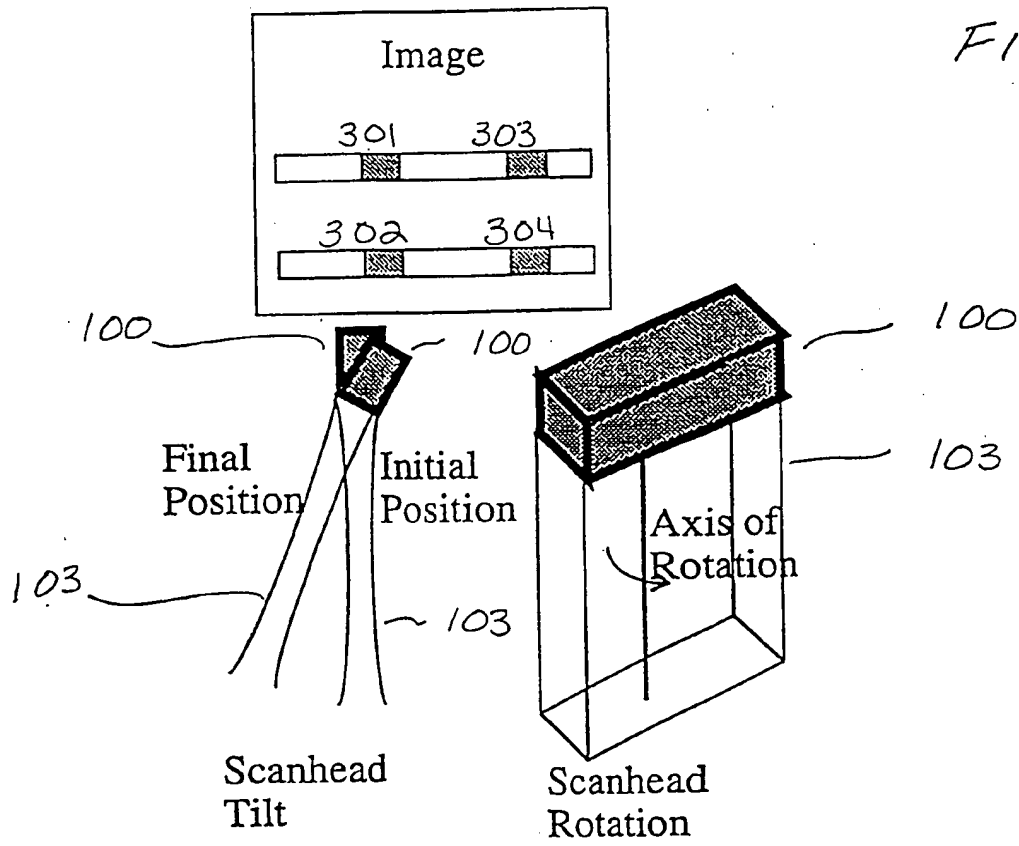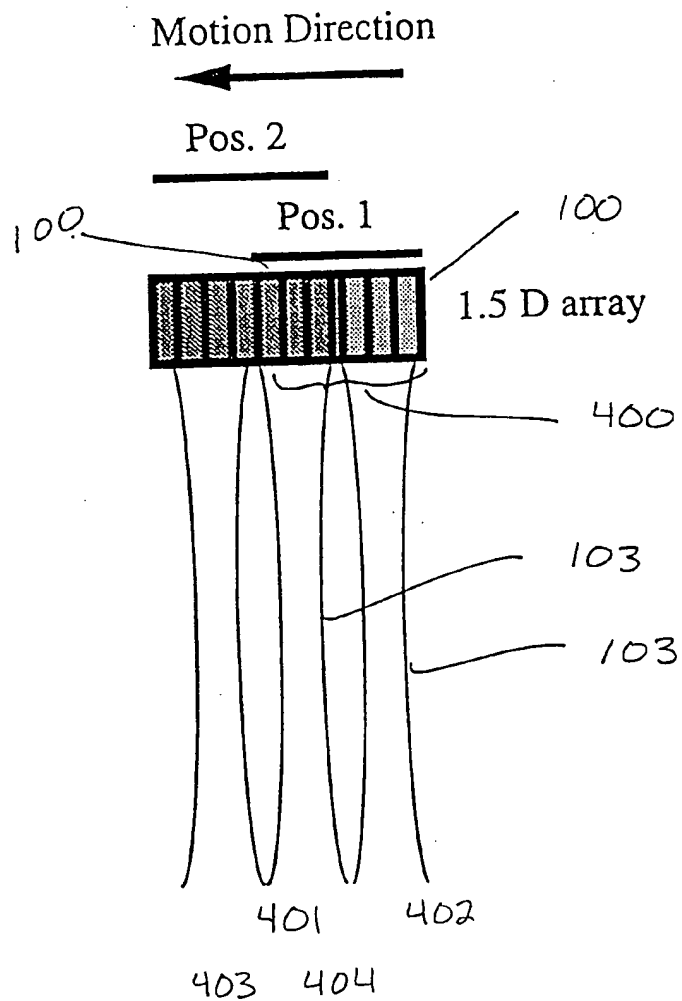7   (i)   utilizing said intersection point to position said data sets.

FIG. 1

DISPLAY
107

Scan Plane

103

100

ULTRASOUND
MACHINE
105

MATERIAL
102

FIG. 2

COLLECT
SCAN DATA   200

DEFINE
DATA
SLICES   205

MEASURE REGION
CORRELATION   210

COMPUTE
RELATIVE
POSITIONAL
DIFFERENCE
VECTOR   215

DETERMINE RELATIVE
3-D POSITIONS OF
DATA SLICES   220

DISPLAY 3-D IMAGE
225

FIG. 3

Motion Direction

FIG. 4

Pos. 2

Pos. 1

100

100

1.5 D array

400

103

103

401   402

403   404

FIG. 5

Two orthogonal 3D scans - irregular image spacing

Top view of plane
intersections

Each grid point is the
maximum correlation value
for the corresponding Amode
lines in the two orthogonal
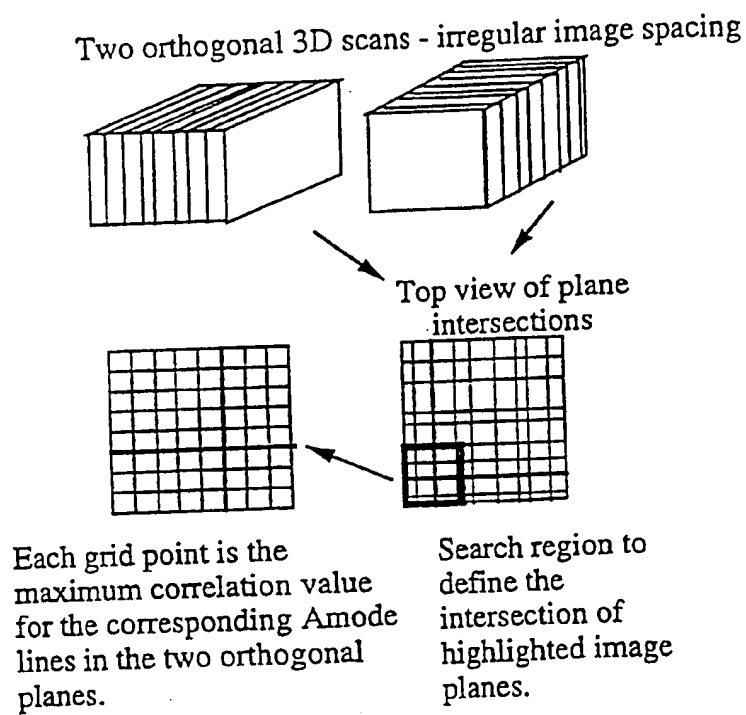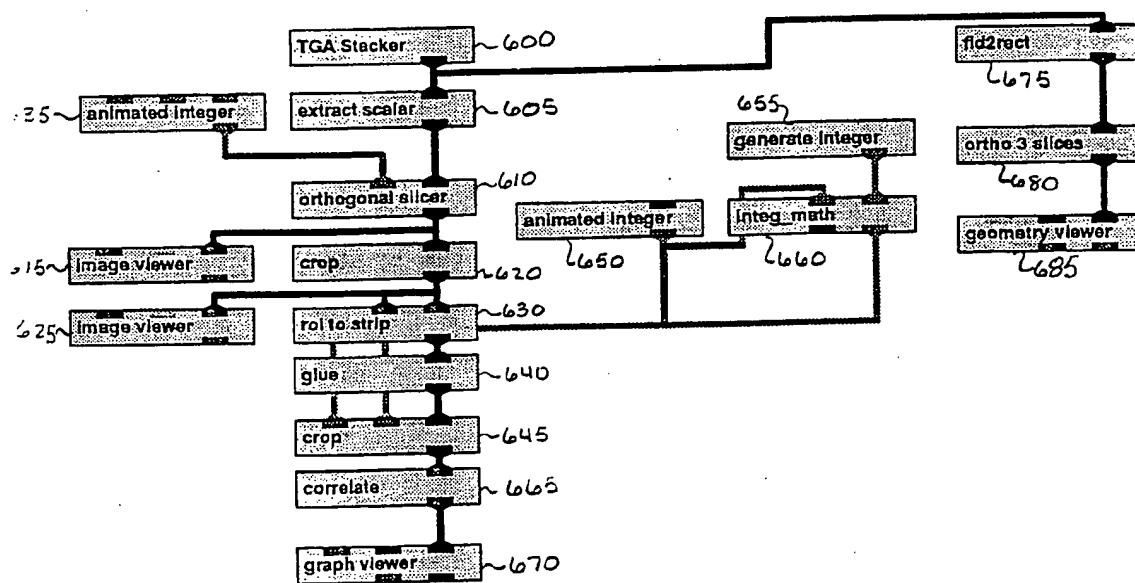planes.

Search region to
define the
intersection of
highlighted image
planes.

- Diagram of A mode correlation for slice positioning.

FIG. 6

Block Diagram
of Software

INTERNATIONAL SEARCH REPORT

A. CLASSIFICATION OF SUBJECT MATTER
IPC(6)   :G06F 15/00; G06T 15/70
US CL   :395/118, 119, 125; 356/35.5
According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

U.S. : 395/114, 118, 119, 120, 124, 125, 125; 356/35.5, 375

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

APS
search terms: speckel (w) (correlat? or decorrelat?)

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	US, A, 5,049,987 (HOPPENSTEIN) 17 September 1991, col.4, line 62 through col.6, line 24.	23-30
A	US, A, 5,287,435 (COHEN ET AL) 15 February 1994.	NONE
A	US, A, 5,000,183 (BONNEFOUS) 19 March 1991.	NONE
A	US, A, 4,322,162 (MCKELVIE ET AL) 30 March 1982.	NONE
A	US, A, 5,061,860 (TAKEMORI) 29 October 1991.	NONE
A	US, A, 5,412,763 (KNOPLIOCH ET AL) 02 May 1995.	NONE
A, P	US, A, 5,426,498 (BRUECK ET AL) 20 June 1995.	NONE

[X] Further documents are listed in the continuation of Box C.   [ ]   See patent family annex.

*	Special categories of cited documents:	"T"	later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
"A"	document defining the general state of the art which is not considered to be part of particular relevance		
"E"	earlier document published on or after the international filing date	"X"	document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
"L"	document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)	"Y"	document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art
"O"	document referring to an oral disclosure, use, exhibition or other means		
"P"	document published prior to the international filing date but later than the priority date claimed	"&"	document member of the same patent family

Date of the actual completion of the international search	Date of mailing of the international search report
28 AUGUST 1996	27 SEP 1996

Name and mailing address of the ISA/US Commissioner of Patents and Trademarks Box PCT Washington, D.C. 20231	Authorized officer HEATHER R. HERNDON
Facsimile No. (703) 305-3230	Telephone No. (703) 305-9701

Form PCT/ISA/210 (second sheet)(July 1992)*

C (Continuation). DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	US, A, 4,967,093 (TAKEMORI) 30 October 1990, col.4, line 10 through col.7, line 12.	1-35